

## Voltage interruption simulator

### VIS 1700\_1



- **AC-Test:** IEC / EN 61000-4-11
- **DC-Test:** IEC / EN 61000-4-29
- **Inrush current measurement** at any phase position  $0^\circ - 360$
- **Automatic AC + DC ramp function** (fig.2), second voltage source not necessary

#### Introduction

The clearly adjustable simulator VIS 1700 can simulate the voltage dips and voltage variations that can be found on supply nets (AC and DC). Different modes of operation are possible:

**Short interruptions 100%:** The supply network of the EUT can be interrupted in any phase position for a defined time (0,1 ms – 9980 ms).

**Voltage dips:** The switching between the rated voltage  $U_1$  and the variable voltage  $U_2$  ( $U_2$  always  $\leq U_1$ ) is always erratic. It can be set at each phase angle of the mains begin or end. The standard test is defined at 40%, 70% and 80%. This test requires the injection of the same phase voltage  $U_2$  at the rear of the device. A step transformer (VIS 740) fulfilled the standard requirement. **Fig. 1**

**Voltage fluctuation:** Fluctuation to an adjustable voltage (0 95 % of  $U_1$ ). The parameters for release time (0,1 – 70 sec.), test time (0,01 – 70 sec.) and recovery time (0,1 – 70 sec.) can be set individually. This is not an additional supply voltage required. **Fig. 2**

**Inrush current:** For each EUT up to max. 16 A rated current (AC) can be measured the inrush current on any phase position ( $0 - 360^\circ$ ).

For oscilloscope analysis there are three BNC jacks on the back side of the unit to examine the parameters voltage, current and trigger.

#### Standard requirements

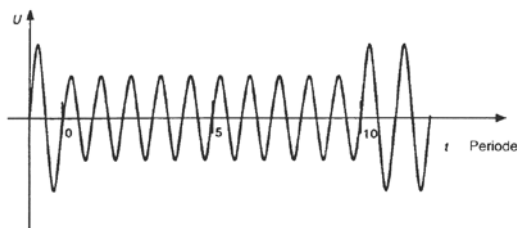


Fig.1: Voltage dips


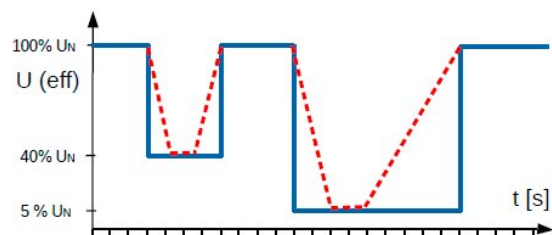


Fig.2: Voltage fluctuation

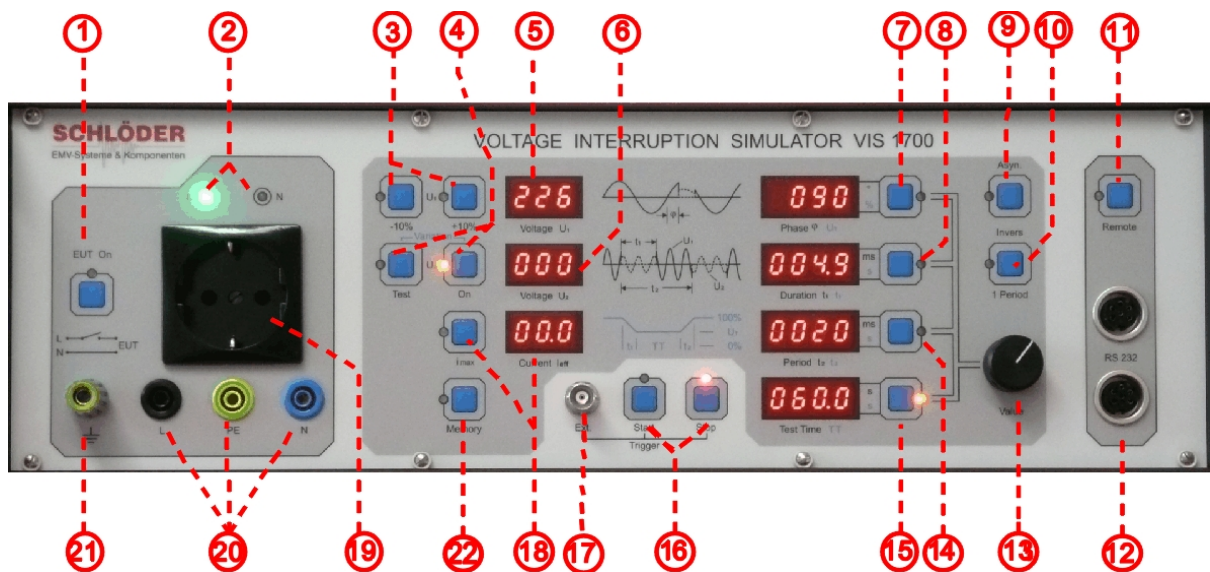

## Technical data

### EUT supply

- ◆ Nominal voltage AC max. 280 V  
DC max. 360 V
- ◆ Nominal current  
Voltage dips (fig. 1)  
AC / DC max. 16 A / 8 A
- Voltage fluctuation (fig. 2)  
AC / DC max. 16 A / 8 A  
*with second voltage source*  
AC / DC max. 16 A / 4 A  
*with automatic ramp function*
- ◆ Phase indication [2] lamp red / green

### Functions:

- [9] Interruptions / voltage variations - synchronous and asynchronous
- [3] Supply voltage  $U_1 = U_N$  : reversing to +10%  $U_N$  and -10%  $U_N$
- [5] Display supply voltage  $U_1$
- [4] Variable voltage  $U_2$  test and  $U_2$  on, activation of the >automatic ramp function< (fig. 2)
- [6] Display variable voltage  $U_2$
- [1] EUT on / off
- [18] Starting inrush current  $I_{max}$  / rated current measurement
- [10] Inverse operation within one period
- [11] Switch for remote control release
- [12] RS 232-interface
- [13] Adjustment for phase angle [7], duration [8], period [14] and test time [15] with digital potentiometer
- [22] MEMORY key

### Functions:

- [7] Phase angle 0 - 359°, step 1°
- [8] Duration  $t_1$  0,1ms - 9980ms
- [14] Period  $t_2$  Asynchronous 5,0ms - 9990ms  
Synchronous 20ms - 9980ms
- [15] Test time 0,1sec - 9990sec, furthermore single event and continuous operation
- [16] Trigger Start- and Stop-key
- [17] Trigger external BNC connector
- [19] EUT connection Protection earth outlet
- [20] Additional lab. jacks
- [21] Ground connection Ground jack at the front side and back side
- ◆ Measurement BNC outputs (on rear) for voltage, current and scope triggering
- ◆ EUT supply " $U_1$ " On rear
- ◆ EUT supply " $U_2$ " On rear (e.g.variac)
- ◆ EUT Fail Trigger-input, on rear

### Common

- ◆ Operation temp. 0 - 40 °C
- ◆ Dimensions 19" housing, 3 HE
- ◆ Weight 13 kg
- ◆ Power supply 100-240V / 47-63Hz / 80VA

### Options:

- ◆ VIS 740 Step transformer 16,0 A  
For voltage fluctuation, fig.2